
EBCD MEDITECH Content Updates – 2025.2 ED Module

Overview

This document is a high-level overview for end user education purposes about significant changes within the ED screens.

First Point of Contact


Current documentation within the First Point of Contact does not take into account if the patient refuses to be masked and/or an isolation bed is unavailable. The new update will include additional fields at the end of the screening to account for these instances.

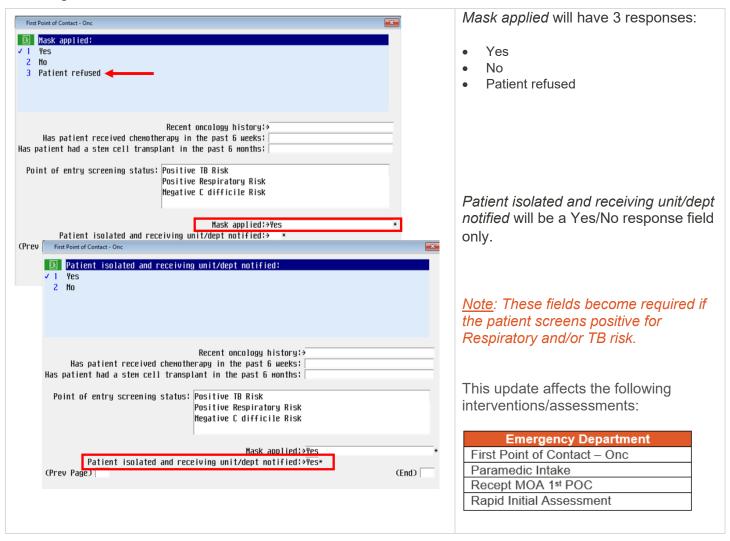

ED Nurse Tracker

The First Point of Contact (FPC) indicator will be retired. The MASK indicator (MSK) will replace the FPC indicator to improve the visibility of the point of entry screening and mask compliance. The MSK indicator adds the ability to identify patients whose screening has not been completed, improving overall compliance and infection control oversight


- A red box displays in the MASK field when point of entry screening has not been completed
- The red box disappears once screening is documented and patient screens negative.
- If patient screens positive, the appropriate MASK (green or red) will display
 - MSK patient screened positive and mask has been documented as applied
 - o MSK patient screened positive and mask has not been applied or the patient refused

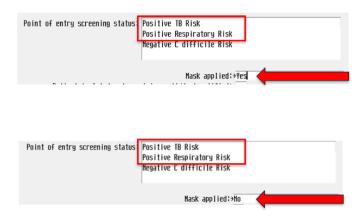

MSK – patient screened positive, and mask has been documented as applied


MSK – patient screened positive, and mask has not been applied or the patient refused

MASK Indicator Tracker Key

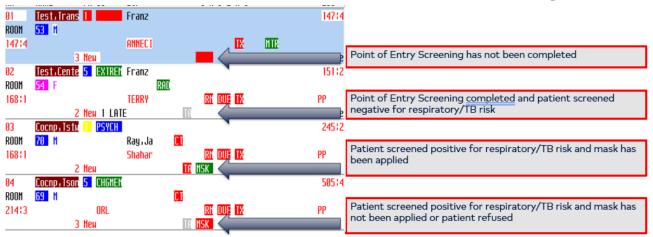


Meals Consumed Intake

Currently, clinicians cannot document when a patient refuses a meal or snack as part of **Intake and Output**. To address this issue, "Patient refused" has been added as a new option, facilitating instances when a patient refuses a meal or snack offered. Information regarding patients who are NPO can be found elsewhere in the medical record.

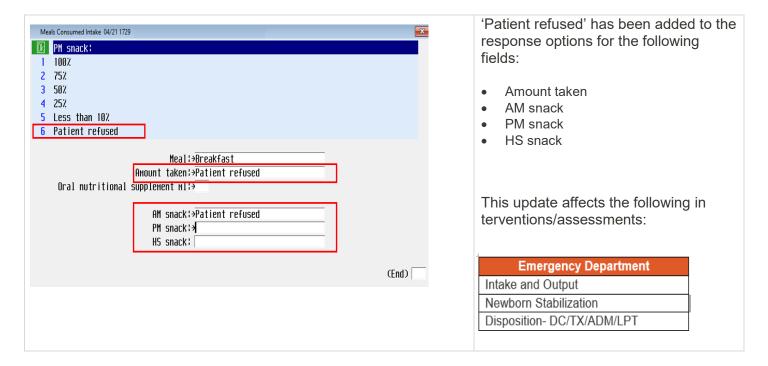


Restraint Documentation


Current documentation allows for the selection of "Quick Release Synthetic" options when non-violent restraints have been ordered. Quick release synthetic restraints should be reserved for violent restraint use only. Future documentation will remove all "Quick Release Synthetic" options from the Non-violent restraint device field.

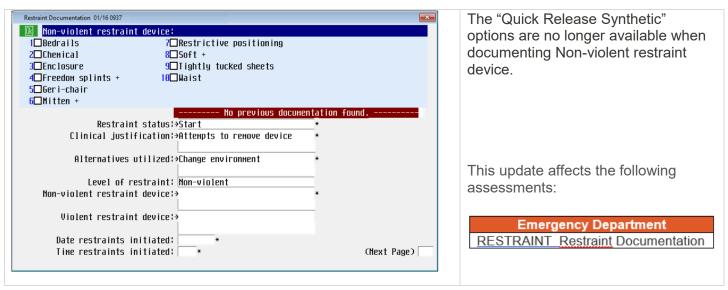

Newborn Resuscitation Efforts


Current documentation for newborns does not allow for nurses to enter CPAP within resuscitation or stabilization efforts. Fields have now been added to include CPAP to accurately reflect care provided.

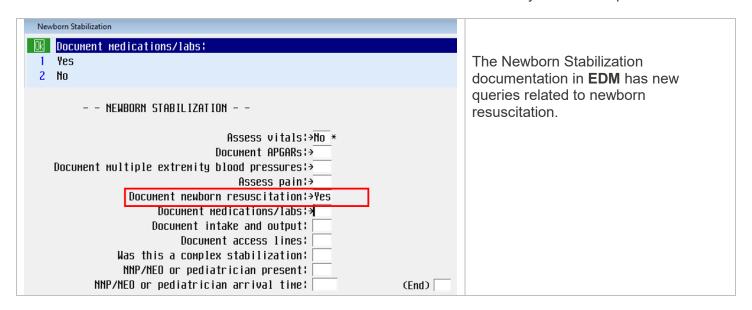

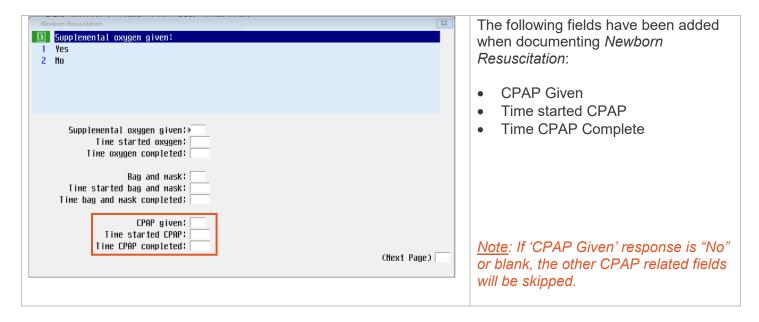

Suicide Screening

The naming convention of the Suicide Assessment is inaccurate as the C-SSRS is not an assessment but a screening tool to evaluate the patient's suicide risk level.

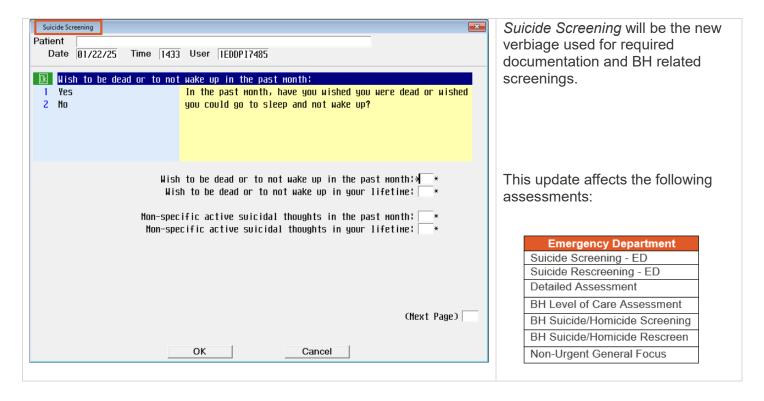

Nursing Support Tracker

Fall Risk indicators have been added underneath the Chief Complaint field:

FR - low risk

🔣 – moderate risk

FR - high risk

